



**USER MANUAL**

**LiVE**  
**JOHANNUS**

*USER MANUAL*  
*LiVE III BDO*

---

Manufacturer Global Organ Group B.V.

Address	Keplerlaan 2 6716 BS EDE
Country	The Netherlands
Telephone	+31 (0)318 63 74 03
E-mail	inform@johannus.com
Website	www.johannus.com
Version	2.5
Date	December 2021
Firmware	starting from version V 3.35, hardware version 'Hw GOG: V3'

**© 2021 Global Organ Group B.V.**

All rights reserved. Nothing in this publication may be reproduced, stored in a data file or made public in any form or in any way either electronically, mechanically by way of photocopying, recording or in any other way without the prior written permission of Global Organ Group B.V.

---

## CONTENTS

<b>1</b>	<b>SAFETY.....</b>	<b>6</b>
1.1	Safety instructions .....	6
1.2	Symbols on the organ .....	7
1.3	Symbols in this manual .....	7
1.4	Transport and storage .....	8
1.5	Cautions and important notes .....	9
1.6	Placement .....	11
1.7	Repairs and data .....	11
1.8	Additional precautions .....	12
<b>2</b>	<b>INSTALLATION .....</b>	<b>13</b>
2.1	Installation and connection .....	13
2.1.1	Installation organ .....	13
2.1.2	Pedal contact calibration .....	14
2.2	Switch on .....	14
<b>3</b>	<b>DESCRIPTION OF THE ORGAN.....</b>	<b>15</b>
3.1	Overview of the components .....	15
3.2	Overview of controls.....	16
3.3	Connect and switch on the peripherals.....	17
3.4	External connections .....	17
<b>4</b>	<b>OPERATION .....</b>	<b>18</b>
4.1	Volume controls.....	18
4.2	Expression pedals .....	18
4.3	Sample banks .....	19
4.3.1	Sample sets .....	19
4.4	Listening positions .....	19
4.5	Stops .....	20
4.5.1	Dynamic stoplist .....	20
4.6	Couplers .....	21
4.7	Accessories .....	22
4.8	Pre-programmed memory locations .....	23
4.9	Capture memory.....	24
4.10	Crescendo pedal .....	24
4.11	Quick Access .....	25
4.11.1	Programming mode crescendo pedal .....	25

---

<b>5</b>	<b>JOHANNUS MENU</b>	<b>26</b>
5.1	Reverb Volume	26
5.2	Fine Tune	27
5.3	Temperaments	27
5.4	Upload Organ	28
5.5	Organ Settings	29
5.5.1	Crescendo	29
5.5.2	Datadump	30
5.5.3	Expression Pedals	31
5.5.4	Intonation	32
5.5.5	Key Volumes	33
5.5.6	MIDI Config	34
5.5.7	Reset	35
5.5.8	Sample Set Version	36
5.6	System Settings	36
5.6.1	Aux In Level	36
5.6.2	Default Ambiance	37
5.6.3	Default Organ	37
5.6.4	Headphones / Aux Out	37
5.6.5	Keyboard Mode	38
5.6.6	Reset	38
5.6.7	Rear Speakers (optional)	39
5.6.8	Side Speakers Level	39
5.6.9	Stop Numbers	40
5.6.10	Tone Control	40
5.6.11	Version	40
<b>6</b>	<b>MAINTENANCE, TROUBLESHOOTING AND WARRANTY</b>	<b>42</b>
6.1	Maintenance	42
6.1.1	Maintenance of the cabinet	42
6.1.2	Maintenance of the manuals	42
6.2	Problems	42
6.3	Warranty	42
<b>7</b>	<b>SPECIFICATIONS</b>	<b>43</b>
7.1	MIDI Implementation Chart	43
7.2	MIDI Specifications	44
7.3	Specifications of Instrument	46

---

# 1 SAFETY

## 1.1 Safety instructions



- To reduce the risk of fire or electric shock, do not expose the organ to liquids, rain or moisture.
- Position the organ on a stable, horizontal surface.
- Connect the organ to a grounded power socket.
- Turn off the organ when it is not in use.
- Do not place the organ in a damp area.
- Follow the instructions and precautionary measures in this user manual.
- Keep this user manual with the organ.
- The organ may only be opened by a technician authorized by Global Organ Group B.V. The organ contains static-sensitive components. The warranty is void if the organ is opened by a non-authorized person.

### **NOTICE**

1. Read these instructions.
2. Keep these instructions.
3. Heed all warnings.
4. Follow all instructions.
5. Do not use this apparatus near water.
6. Clean only with a dry cloth.
7. Do not block any of the ventilation openings.  
Install in accordance with the manufacturer's instructions.
8. Do not install near any heat sources such as radiators, heat registers, stoves, or other apparatus (including amplifiers) that produce heat.
9. Do not defeat the safety purpose of the polarized or grounding-type plug. A polarized plug has two blades with one wider than the other. A grounding type plug has two blades and a third grounding prong. The wide blade or the third prong are provided for your safety. If the provided plug does not fit into your outlet, consult an electrician for replacement of the obsolete outlet.
10. Protect the power cord from being walked on or pinched particularly at plugs, convenience receptacles, and the point where they exit from the apparatus.
11. Only use attachments/accessories specified by the manufacturer.
12. Unplug this apparatus during lightning storms or when unused for long periods of time.
13. Refer all servicing to qualified service personnel. Servicing is required when the apparatus has been damaged in any way, such as power-supply cord or plug is damaged, liquid has been spilled or objects have fallen into the apparatus, the apparatus has been exposed to rain or moisture, does not operate normally, or has been dropped.

## 1.2 Symbols on the organ

 **CAUTION**  
RISK OF ELECTRIC SHOCK  
DO NOT OPEN 

**注意**  
感電の恐れがあります キャビネットをあけないでください

**警告**  
为了避免触电, 请勿自行拆开机壳, 内部无用户自行维修的机件。请交乐兰公司指定维修点进行维修事宜。

**경고** 전기쇼크위험 - 열지 마시오.

**ATTENTION:** RISQUE DE CHOC ELECTRIQUE NE PAS OUVRIR

**WARNING:** TO REDUCE THE RISK OF FIRE OR ELECTRIC SHOCK, DO NOT EXPOSE THIS APPLIANCE TO RAIN OR MOISTURE.

**AVERTISSEMENT:** POUR RÉDUIRE LE RISQUE D'INCENDIE OU DE CHOC ÉLECTRIQUE, N'EXPOSEZ PAS CET APPAREIL À LA PLUIE OU À L'HUMIDITÉ.



- Laite on liitettävä suojamaadoituskoskettimilla varus ettuun pistorasiaan.
- Apparatets stikprop skal tilsluttes en stikkontakt med jord, som giver forbindelse til stikproppens jord
- Apparatet må tilkoples jordet stikkontakt.
- Apparaten skall anslutas till jordat uttag.

THIS DEVICE COMPLIES WITH PART 15 OF THE FCC RULES. OPERATION IS SUBJECT TO THE FOLLOWING TWO CONDITIONS: (1) THIS DEVICE MAY NOT CAUSE HARMFUL INTERFERENCE, AND (2) THIS DEVICE MUST ACCEPT ANY INTERFERENCE RECEIVED, INCLUDING INTERFERENCE THAT MAY CAUSE UNDESIRE OPERATION.

CAN ICES-3(B)/NMB-3(B)

仅适用于非热带气候条件下安全使用  
仅适用于海拔2000m以下地区安全使用



**Warning:** The exclamation point within an equilateral triangle is intended to alert the user to the presence of important operating and maintenance (servicing) instructions in the literature accompanying the product.



The lightning flash with arrowhead symbol, within an equilateral triangle, is intended to alert the user to the presence of uninsulated "dangerous voltage" within the product's enclosure that may be of sufficient magnitude to constitute a risk of electric shock to persons.



**Warning for static-sensitive components.** To prevent damage to electronic parts from static electricity, be sure to discharge any static electricity from your own body before handling / touching the instrument.

## 1.3 Symbols in this manual



Caution, Warning or important information



Do not, or forbidden to do



Note

---

## 1.4 Transport and storage

Pay attention to the following during transport and storage:

- Remove the music desk and the pedal board from the organ, before transport.
- Store in an area with 40% to 60% relative humidity.  
Do not store in area's e.g. baths, washrooms, on wet floors, expose to steam or smoke, salt, humid, rain, moisture, dusty or sandy locations.
- Minimum temperature within the storage area: 0°C
- **Do not expose the Organ to direct sunlight (UV)**, do not place it near devices that radiate heat, or otherwise subject to temperature extremes. Also, do not allow lighting devices that normally are used while their light source is very close to the Organ (such as a piano light), or powerful spotlights to shine upon the same area of the Organ for extended periods of time. Excessive heat can deform or discolor the Organ.
- **Do not allow rubber, vinyl or similar materials to remain on this Organ for long periods of time.** Such objects can discolor or otherwise harmfully affect the finish.
- **Do not paste stickers, decals, or the like to this instrument.** Peeling such matter off the instrument may damage and or discolor the exterior finish.
- Do not bend the power cord or place heavy objects on it.
- **Don't allow foreign objects or liquids to enter Organ;**  
**Never place containers with liquid on Organ;** Do not put anything that contains water on this Organ. Also, avoid the use of insecticides, perfumes, alcohol, nail polish, spray cans, etc., near the Organ. Swiftly wipe away any liquid that spills on the Organ using a dry, soft cloth. Never use benzene, thinners, alcohol or solvents of any kind, to avoid the possibility of discoloration and/or deformation.
- **Unplug the power cord from the outlet before cleaning.** Before cleaning the Organ, turn it off and unplug the power cord from the outlet. To clean the Organ, use a dry, soft cloth; or one that is slightly dampened. Try to wipe the entire surface using an equal amount of strength, moving the cloth along with the grain of the wood. Rubbing too hard in the same area can damage the finish.
- **Do not open. Do not disassemble or modify by yourself**
- **Avoid climbing on top of the Organ, or placing heavy objects on it, nor on top of the keyboard nor pedal board. This can lead to dangerous situations** - such as tilting / tipping over - shearing / falling off of heavy objects. This can also lead to malfunctions - such as keys ceasing to produce sound.
- **Do not bend, drop, strong shock or vibration.**
- Never strike or apply strong pressure to the display.
- **Cautions when moving this Organ:** Since this product is very heavy, you must make sure that a sufficient number of people are on hand to help, so you can lift and move it safely, without causing strain. Make sure to have a firm grip, to protect yourself from injury and the instrument from damage. If you need to move the instrument, consult with your retailer, or Global Organ Group B.V.



---

## 1.5 Cautions and important notes

### Indoor use only.

**Connect the power cord to an outlet of the correct voltage.** The Organ should be connected to a power supply only of the type described as marked under the keyboard deck of Organ.



**Make sure that the power cord is grounded.** Connect mains plug of this model to a mains socket outlet with a protective earthing connection.



**Do not connect or disconnect the power cord with wet hands.** Never handle the power cord or its plugs with wet hands when plugging into, or unplugging from, an outlet.



**Turn off the Organ if an abnormality or malfunction occurs.** Immediately turn the Organ off, remove the power cord from the outlet, and request servicing by your retailer, or Global Organ Group B.V., when:



- The power-supply cord or the plug has been damaged; or
- If smoke or unusual odor occurs; or
- Objects have fallen into, or liquid has been spilled onto the Organ; or
- The Organ has been exposed to rain (or otherwise has become wet); or
- The Organ does not appear to operate normally or exhibits a marked change in performance.

**Do not use the organ overseas in foreign countries.** Before using the Organ in a foreign country, consult with your retailer, or Global Organ Group B.V.



**Presence of children.** For their safety, adults should make sure that children under the age of 16 use the instrument properly and that the organ is in a stable position. An adult should always be present to supervise and guide any use by a child. Due to the weight of the instrument, it is recommended that it be securely fixed to the wall or floor by a professional to prevent tipping over. This is despite the fact that all safety precautions have been taken to avoid accidents.



**Do not connect this Organ to same electrical outlet that is being used by an electrical appliance that is controlled by an inverter or a motor** (such as a refrigerator, washing machine, microwave oven, or air conditioner). Depending on the way in which the electrical appliance is used, power supply noise may cause this Organ to malfunction or may produce audible noise. If it is not practical to use a separate electrical outlet, connect a power supply noise filter between this Organ and the electrical outlet.



**Do not share an outlet with an unreasonable number of other devices.** Do not force the Organ's power-supply cord to share an outlet with an unreasonable number of other devices. Be especially careful when using extension cords—the total power used by all devices you have connected to the extension cord's outlet must never exceed the power rating (watts/amperes) for the extension cord. Excessive loads can cause the insulation on the cord to heat up and eventually melt through - therefore always completely unwind an extension cord.



**To prevent malfunction and equipment failure, always make sure to turn off the power on all your equipment before you make any connections.**





Although the LCD and LEDs are switched off when the Organ is turned off, this does not mean that the Organ has been completely disconnected from the source of power. If you need to turn off the power completely, first turn off the Organ's switch, then unplug the power cord from the power outlet. For this reason, the outlet into which you choose to connect the power cord's plug should be one that is within easy reach and readily accessible.



If there is a possibility of lightning strike, disconnect the power cord from the outlet. Whenever you suspect the possibility of lightning in your area, pull the plug on the power cord out of the outlet.



**Periodically clean the power cord's plug.** At regular intervals, you should unplug the power plug and clean it by using a dry cloth to wipe all dust and other accumulations away from its prongs. Also, disconnect the power plug from the power outlet whenever the Organ is to remain unused for an extended period of time. Any accumulation of dust between the power plug and the power outlet can result in poor insulation and lead to fire.



**The settings you were editing will be lost when the Organ is turned off.** If you want to keep your settings, you must save your settings before turning the Organ off.



**Place in a well ventilated location.** The Organ should be located so that its location or position does not interfere with its proper ventilation.



**Manage cables for safety.** Try to prevent cords and cables from becoming entangled. Also, all cords and cables should be placed so they are out of the reach of children.



**Grasp the plug when connecting or disconnecting the power cord.** Always grasp only the plug on the power-supply cord when plugging into, or unplugging from, an outlet.



**Precautions concerning use of bench.** When using the bench, please observe the following points:



- Do not allow two or more persons to sit on the bench.
- Do not adjust the height while sitting on the bench.



**Do not remove the speaker grille and speaker.** Do not remove the speaker grille and speaker by any means. Speaker not user replaceable. Shock hazardous voltages and currents are present inside the enclosure.



**Disconnecting power from AC mains.** To completely disconnect this instrument from the AC mains, disconnect the power supply cord plug from the AC receptacle.



**The power supply cord and/or main power switch must be accessible.** The mains plug of the power supply cord shall remain readily accessible. Or, the power switch must be accessible. The main power switch is the main power disconnect device for this Organ. Therefore, the power switch shall be readily accessible.



**Do not use internal connections.** Do not connect, do not use internal connections for optional external speakers by yourself. Refer all servicing to your retailer, or Global Organ Group B.V.



---

## 1.6 Placement

- Using the Organ near power amplifiers (or other equipment containing large power transformers) may induce hum. To alleviate the problem, change the orientation of this Organ; or move it farther away from the source of interference.
- This device may interfere with radio and television reception. Do not use this device in the vicinity of such receivers.
- Noise may be produced if wireless communications devices, such as cell phones, are operated in the vicinity of this Organ. Such noise could occur when receiving or initiating a call, or while conversing. Should you experience such problems, you should relocate such wireless devices so they are at a greater distance from this Organ, or switch them off.
- **Do not expose the Organ to direct sunlight**, place it near devices that radiate heat, or otherwise subject it to temperature extremes. Also, do not allow lighting devices that normally are used while their light source is very close to the Organ (such as a piano light), or powerful spotlights to shine upon the same area of the Organ for extended periods of time. Excessive heat can deform or discolor the Organ.
- **Do not allow rubber, vinyl, or similar materials to remain on this Organ for long periods of time.** Such objects can discolor or otherwise harmfully affect the finish.
- **Do not allow objects to remain on top of the keyboard or pedal board.** This can be the cause of malfunction, such as keys ceasing to produce sound.
- **Do not paste stickers, decals, or the like to this instrument.** Peeling such matter off the instrument may damage the exterior finish.
- **Do not put anything that contains water on this Organ.** Also, avoid the use of insecticides, perfumes, alcohol, nail polish, spray cans, etc., near the Organ. Swiftly wipe away any liquid that spills on the Organ using a dry, soft cloth.
- Due to the weight of the instrument, it is recommended to attach the instrument securely to the wall or floor by a professional, to avoid tipping. This, although all safety measures have been taken to avoid any accident.



## 1.7 Repairs and data





Please be aware that all data contained in the Organ's memory may be lost when the Organ is sent for repairs. Important data should always be stored on USB stick (see ['Datadump' chapter 5.5.2](#)), or written down on paper (when possible).



During repairs, due care is taken to avoid the loss of data. However, in certain cases (such as when circuitry related to memory itself is out of order), we regret that it may not be possible to restore the data, and Global Organ Group B.V. assumes no liability concerning such loss of data. Refer all servicing to your retailer, or Global Organ Group B.V.

---

## 1.8 Additional precautions

- Please be aware that the contents of memory can be irretrievably lost as a result of a malfunction, or the improper operation of the Organ. To protect yourself against the risk of losing important data, we recommend that you periodically write down important setting data on (several) USB-sticks, see chapter [‘Datadump’ 5.5.2](#), or on paper (when possible). 
- Unfortunately, it may be impossible to restore the contents of data that was stored in the Organ’s memory once it has been lost. Global Organ Group B.V. assumes no liability concerning such loss of data. 
- Use a reasonable amount of care when using the Organ’s buttons, sliders, or other controls; and when using its jacks and connectors. Rough handling can lead to malfunctions. 
- Never strike or apply strong pressure to the display.
- A small amount of heat will radiate from the Organ during normal operation.
- To prevent possible hearing damage, do not listen at high volume levels for long periods. This Organ, either alone or in combination with an amplifier and headphones or speakers, may be capable of producing sound levels that could cause permanent hearing loss. Do not operate for a long period of time at a high volume level, or at a level that is uncomfortable. If you experience any hearing loss or ringing in the ears, you should immediately stop using the Organ, and consult an audiologist. 
- To avoid disturbing others nearby, try to keep the Organ’s volume at reasonable levels. You may prefer to use headphones, so you do not need to be concerned about those around you.
- When you need to transport the Organ, pack it in shock-absorbent material. Transporting the Organ without doing so can cause it to become scratched or damaged, and could lead to malfunction.
- Do not apply undue force to the music stand while it is in use.
- Some connection cables contain resistors. Do not use cables that incorporate resistors for connecting to this Organ. The use of such cables can cause the sound level to be extremely low, or impossible to hear. For information on cable specifications, contact the manufacturer of the cable.
- Due to the structural design of this instrument, small pets or other animals could end up getting trapped inside it. If such a situation is encountered, you must immediately turn off the Organ and disconnect the power cord from the outlet. You should then consult with the retailer from whom the instrument was purchased, or contact Global Organ Group B.V.
- The explanations in this manual include illustrations that depict what should typically be shown by the display.

Note, however, that your Organ may incorporate a newer, enhanced version of the system (e.g., includes newer sounds), so what you actually see in the display may not always match what appears in the manual.

---

## 2 INSTALLATION

### 2.1 Installation and connection

#### 2.1.1 Installation organ




1. Position the organ on a stable, horizontal surface.
2. Lean the organ slightly backward.
3. Slide the pedal board (C) against the organ.
4. Set the organ upright.
5. Place the organ bench (B) over the pedal board (C).
6. Make sure the voltage of the organ matches the voltage of the main. See the serial plate (A).
7. Connect the organ to a grounded power socket.
8. Perform a pedal contact calibration. See § 2.1.2.

### 2.1.2 Pedal contact calibration

Perform a pedal contact calibration after installing or moving an organ.  
First activate one or more pedal stops, make sure the organ produces sound.

1. Check if pedal board is tightly pressed against the organ and the organ stands on a stable, horizontal surface. Check if each pedal key produces sound at the desired key depth. Follow steps below when the pedal board appears un-even or partially not functioning:
2. Remove the organ bench and slide the pedal board away from the organ. It may be necessary to lean the organ slightly backwards to do this.
3. Now the pedal position set screws on both sides of the organ are visible, see image below. These set screws are to adjust the pedal key depth.

*Image LiVE III BDO - set screws are to adjust the pedal key depth*

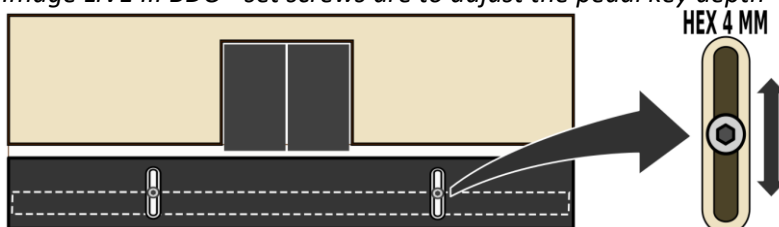

Loosen the set screws a little to adjust the positions a little upwards, or downwards. This moves the magnetically sensitive pedal contact position relative to the pedal key magnets of the pedal board. Tighten the set screws at the new pedal key depth position – and remember the set positions.

4. Lean the organ slightly backward to slide the pedal board against the organ and set the organ upright afterwards.
5. If you want, place the organ bench over the pedal board.
6. Repeat step 1 to check the difference and repeat steps 2 to 6 when further improvement is needed.

## 2.2 Switch on

Switch on the organ with the on/off switch at the right, underneath the manuals. Wait several seconds. Starting the control functions and the settings will take some time.


The lights of standard set functions light up. The settings appear on the display.

Utrecht, Bätz Location Organ Console		
Mem : 1	■	■
Trans : 0		
Tune : 431Hz		
Temp : Original		
Cresc : Off	I/II/Pd	III

---


### 3 DESCRIPTION OF THE ORGAN

#### 3.1 Overview of the components

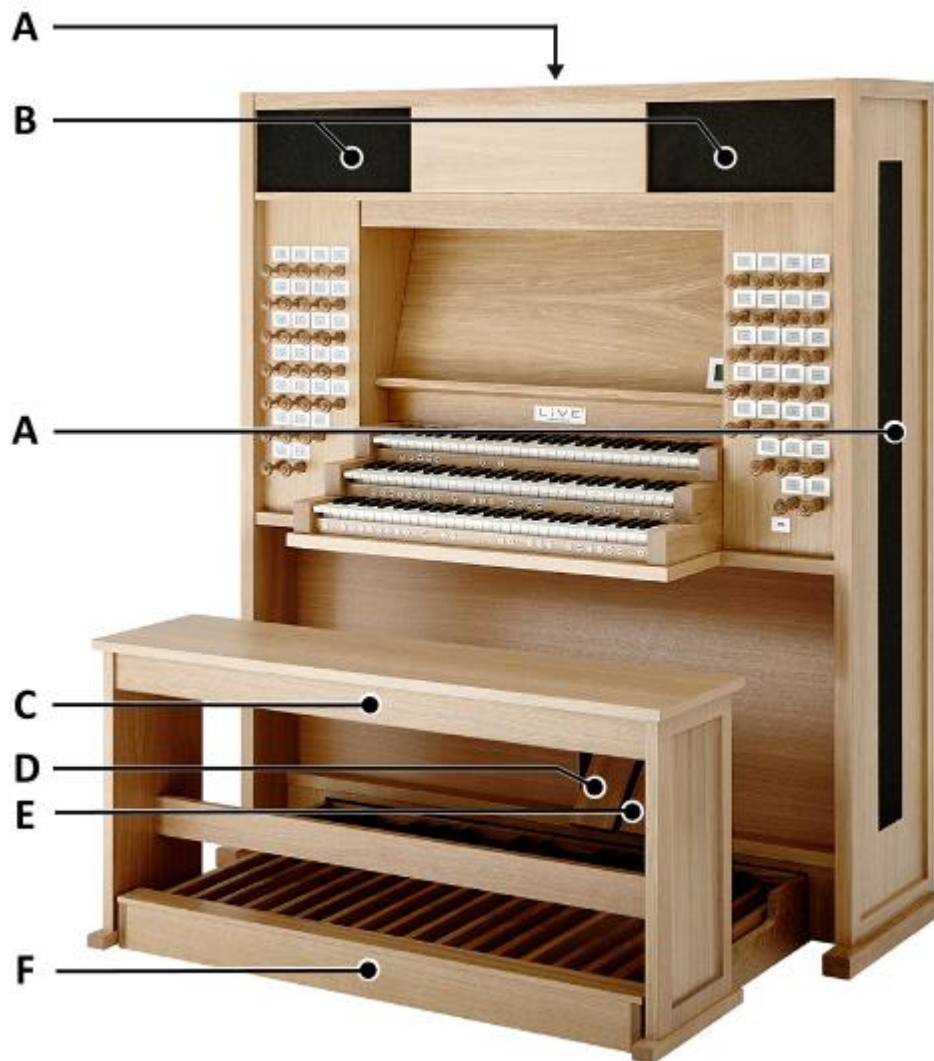

- A Surround loudspeakers
- B Loudspeakers
- C Organ bench
- D Swell pedal
- E Crescendo pedal
- F Pedal board

### 3.2 Overview of controls

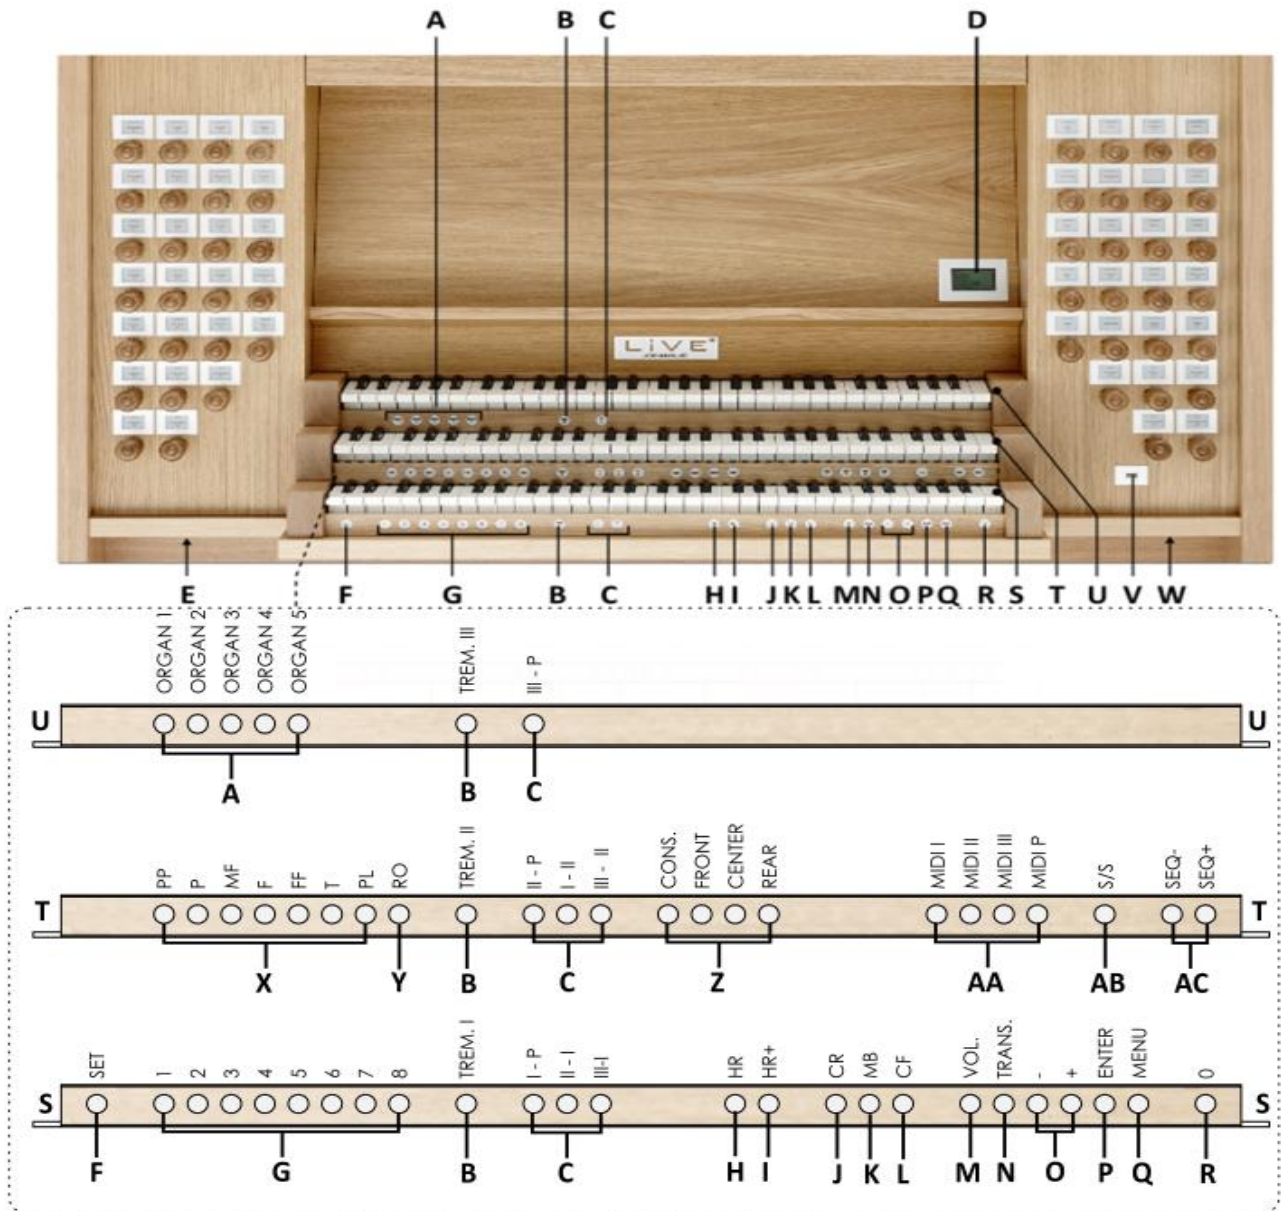

- |                                        |                                                                    |
|----------------------------------------|--------------------------------------------------------------------|
| <b>A</b> Sample banks (Organ 1 to 5)   | <b>P</b> ENTER                                                     |
| <b>B</b> Tremulants Manuals I, II, III | <b>Q</b> MENU                                                      |
| <b>C</b> Couplers                      | <b>R</b> 0: Cancel                                                 |
| <b>D</b> Display                       | <b>S</b> Manual I                                                  |
| <b>E</b> Headphones connection         | <b>T</b> Manual II                                                 |
| <b>F</b> SET                           | <b>U</b> Manual III                                                |
| <b>G</b> Capture memory locations      | <b>V</b> USB port                                                  |
| <b>H</b> HR: Hand Registration         | <b>W</b> On/Off switch (AC-Mains power switch) bottom of the keyed |
| <b>I</b> HR+: Hand Registration +      | <b>X</b> Pre-programmed memory locations                           |
| <b>J</b> CR: Crescendo                 | <b>Y</b> RO: Reeds Off                                             |
| <b>K</b> MB: Manual Bass               | <b>Z</b> Listening Positions                                       |
| <b>L</b> CF: Cantus Firmus             | <b>AA</b> MIDI registers                                           |
| <b>M</b> VOL.: General Volume          | <b>AB</b> S/S: All Swells to Swell                                 |
| <b>N</b> TRANS.: Transposer            | <b>AC</b> SEQ- and SEQ+ pistons                                    |
| <b>O</b> - and + pistons               |                                                                    |

### 3.3 Connect and switch on the peripherals

You can connect peripherals (for example, a MIDI device) to the organ.




Follow the instructions provided in the documentation for the peripheral.

1. Switch off the organ and the peripheral.
2. Connect the peripheral to the organ.
3. Switch on the peripheral.
4. Switch on the organ.

### 3.4 External connections

The following external connections are on the left backside of the organ:

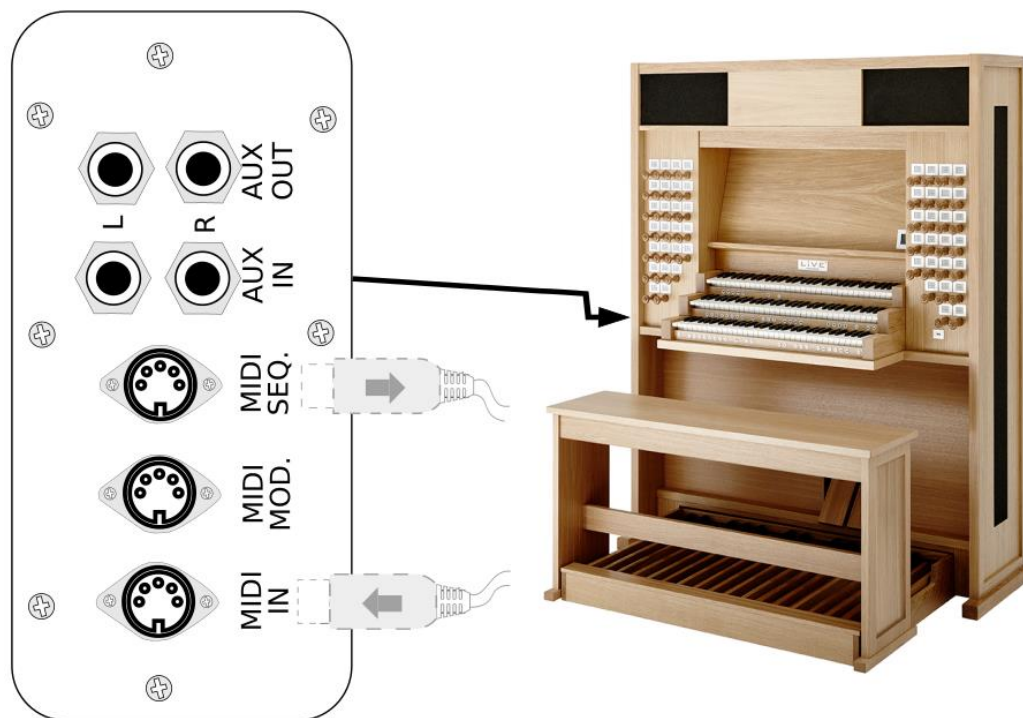

**MIDI IN:** An input for receiving MIDI codes from other devices.

**MIDI MOD:** A programmable MIDI output for connecting a sound module or expander, for example.

**MIDI SEQ:** A non-programmable MIDI output for connecting the Johannus MIDI Sequencer+ or PC (with the optional Johannus Intonat program), for example.

**AUX IN:** A stereo audio input for playing the sound of an external device through the amplifiers of the organ. For example, an expander connected to the organ through the MIDI MOD can be played through the instrument's loudspeakers.

**AUX OUT:** A stereo audio output for connecting an external device (amplifier or recording device, for example).



---

The following external connections are on the front side of the organ:

**Headphone connection:** This connection for a (stereo) headphone, Johannus Pure Audio™, is suited for a headphone with an impedance of 30 Ω or more (see headphone specifications). Location of the connection: see §3.2 Overview of Controls, point E.



When the headphone is used, the loudspeakers of the organ are switched off automatically.

**USB port:** This connection is suited for the connection of an USB stick up to 32GB with a (pre-formatted) **FAT32 file system**, for example for uploading sample sets of new pipe organs. Location of the connection: see §3.2 Overview of Controls, point V.

## 4 OPERATION

### 4.1 Volume controls

**General Volume:** The volume of the organ can be adjusted with the VOL.-piston (0-100%).

1. Press the VOL.-piston.
2. Use the – and + pistons to set the volume. The settings appear on the display.



Adjusting the volume is only possible as long as the VOL.-piston is lit.



When the volume change needs to be saved, press the ENTER-piston in the time the VOL.-piston is lit.

### 4.2 Expression pedals

In the standard version the organ has two expression pedals. One is configured as a swell pedal for Manual III, and one is configured as a crescendo pedal. With use of the Johannus Menu, the function of the expression pedals can be changed, see §5.6.3 Expression Pedals.

Using an expression pedal which is set as a swell pedal will, next to the volume, also change the timbre of the stops. By this the effect of the swell box shutters of a pipe organ is simulated.

---

## 4.3 Sample banks

The Johannes LiVE III is a fully fledged digital organ that uses sample sets, through which you can play numerous international pipe organs. The organ is equipped with the LIVEverb II™ system. This system produces a natural reverb using recordings of the acoustics of existing international pipe organs.

### 4.3.1 Sample sets

Sample set(s) are stored on one or more USB sticks, containing a professional, authentic set of recordings from an actual pipe organ. You can upload sample sets for dozens of international pipe organs on the Johannes III.

These sample sets contain a large number of unique stops for these organs. The result is that every sample set for the Johannes LiVE III contains minimal 50 stops, most of which come from the original pipe organ, the rest being supplementary stops in the spirit of and complementary to the character of the pipe organ concerned.

The LiVE III organ has enough capacity to store five complete pipe organs. Practically speaking that means that you can copy five USB sticks containing full recordings into the Johannes LiVE's memory. With the pistons ORGAN 1 to ORGAN 5 you can easily switch between pipe organs:

- Press the ORGAN piston once to see the overview of available sample sets.
- Press the ORGAN piston twice to switch to another pipe organ that is saved at that location. The organ stop names will change on the small dynamic displays above each stop individually. See §3.2 Overview of Controls, point A.

If you have more than five sample sets, you can easily reload a new one by overwriting one of the existing sample sets. If you want to go back to your original selection, simply reload the sample set that you overwrote. The sample sets can be uploaded into the organ with an USB stick. See §5.4 Upload Organ.

#### Ordering sample sets

When you purchase a Johannes LiVE III, it comes with two sample sets. New pipe organ recordings can be ordered individually from your dealer.



The sets are protected by a unique code, so they can only be used on your own organ.

## 4.4 Listening positions

The Sampled Listening Positions™ is a function which works with the LIVEverb II™ to position the organ sound in the church. It lets you choose where to sit in the church to enjoy the sound of the organ.

The Johannes LiVE gives you essentially four different recordings for each organ: the organ bench, about ten meters from the front, the middle of the church, and

---

the back of the church. A pipe organ sounds very different from all those different locations. From the organ bench, direct sound dominates the experience, with reverb in the background; from the middle of the church, in contrast, sound and reverb meld together far more seamlessly.

There is choice out of four locations:

- Location Organ Console (CONS.) you are listening at the console of the organ
- Location Front (FRONT) you are listening in front of the church
- Location Center (CENTER) you are listening in the middle of the church
- Location Rear (REAR) you are listening at the back of the church

The pistons CONS., FRONT, CENTER and REAR allow you to choose where to listen to enjoy the sound of your organ. The chosen listening position appears on the display. See §3.2 Overview of Controls, point Z.


## 4.5 Stops

The stops are activated via draw stops, pre-programmed memory locations, capture memory locations or the crescendo pedal.

### 4.5.1 Dynamic stoplist

The small dynamic displays above each stop individually, show the stop names of the organ which is selected. When you switch to a different sample set with pistons ORGAN 1 to ORGAN 5, the stop names immediately changes to the stop names of the other selected organ. See 5.6.8 for Sample Set version.

*Image – On the LiVE III small dynamic displays show the real pipe organ stop names of the selected ORGAN. The solid wooden drawknobs are lightened when activated (optional, not in image below).*

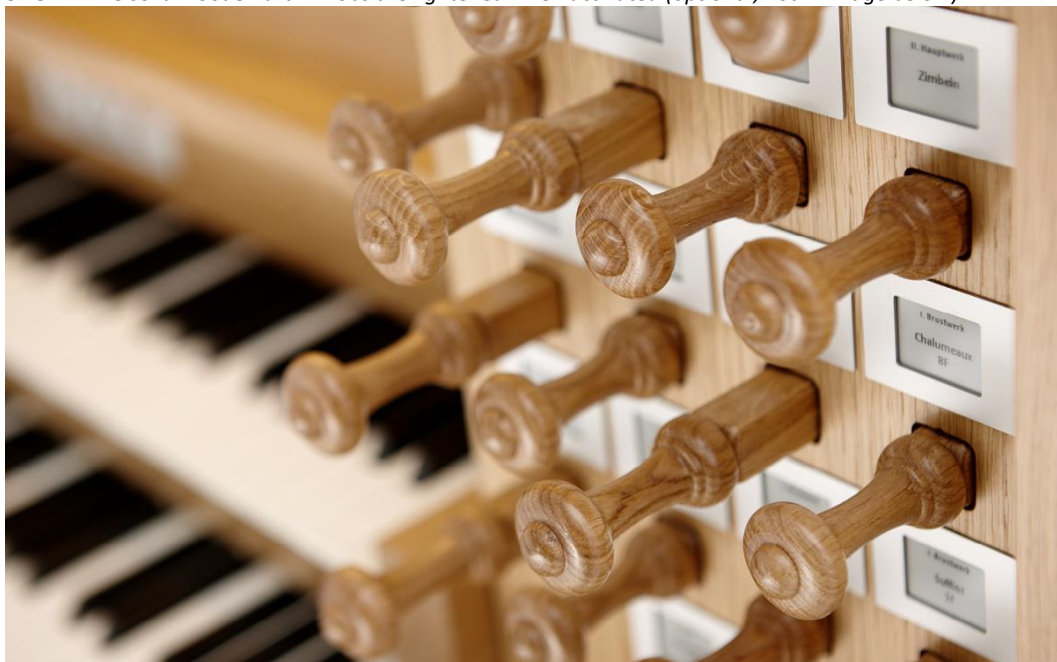

The designation of the stop groups are different per sample set. The stops are divided into the following main groups:

- 
- Pedal (P):** Activates the stops of the Pedal.  
**Manual I:** Activates the stops of Manual I.  
**Manual II:** Activates the stops of Manual II.  
**Manual III:** Activates the stops of Manual III.



The contrast of the dynamic displays might reduce if the organ is inactive for an extended period of time. When switching on the organ, the displays get back to their original contrast.

## 4.6 Couplers

### **Manual couplers:**

MANUAL I – MANUAL II (I-II):

Couples all keys of Manual I to Manual II.

MANUAL II – MANUAL I (II-I):

Couples all keys of Manual II to Manual I

MANUAL III – MANUAL II (III-II):

Couples all keys of Manual III to Manual II.

MANUAL III – MANUAL I (III-I):

Couples all keys of Manual III to Manual I.

### **Pedal couplers:**

MANUAL I – PEDAL (I-P):

Couples all keys of Manual I to the Pedal.

MANUAL II – PEDAL (II-P):

Couples all keys of Manual II to the Pedal.

MANUAL III – PEDAL (III-P):

Couples all keys of Manual III to the Pedal.

The location of the stops per division vary from sample set, therefore the couplers are indicated by roman numerals.

---

## 4.7 Accessories

### Reeds Off (RO):

Reeds Off is a function to switch off all reed stops simultaneously. As long as this piston is lighted, no reed stops can be activated. When this function is switched off, the reed stops that were on are activated again. Activate the Reeds Off with the RO-piston.

### Sequence - and + (SEQ-, SEQ+):

Sequence is a function for sequential selecting capture memory locations.

1. Select a capture memory location to start.  
(for example level 2, location 2)
2. Use the SEQ- or SEQ+ pistons to select the previous or next capture memory location 1-8.
3. When using SEQ+ on position 8, it switches to the next memory bank, position 1.

### All Swells to Swell (S/S):

All Swells to Swell transforms the expression pedal for Manual III, to a swell pedal for the whole organ. Activate the All Swells to Swell with the S/S-piston.



If no expression pedal is configured as a swell pedal for Manual III, the S/S-piston cannot be activated.

### Hand Registration (HR)

Only when the HR-piston is activated, you will be able to register manually.



If you are unable to hear an organ sound, after you have pulled a draw stop and pressed a key, please check if the HR-piston is activated.

### Hand Registration + (HR+)

Only when the HR+ piston is activated, you can join your own registration to the fixed- (PP to T and PL), or the capture memory combinations (1 – 8 and Mem. 1 - 50).

### Manual Bass (MB):

Couples the Pedal monophonic to Manual II. Only the lowest key that is played on Manual II is coupled from the Pedal to Manual II.

If only the lowest key of a chord is released, the pedal key activated by the Manual Bass function is dropped until a new lowest key is played.

Activate the Manual Bass with the MB-piston.



It is advisable not to use the Manual Bass while playing the pedal board to avoid double bass tones.

### Cantus Firmus (CF):

Cantus firmus: Latin for 'fixed voice' or in organs 'solo voice' or 'melody coupler'.

Couples Manual III monophonic to Manual II. Only the highest key that is played on Manual II is coupled from Manual III to Manual II.

With use of a solo registration on Manual III in this way a solo is heard while playing only on Manual II.

If only the highest key of a chord is released, the key activated by the Cantus Firmus function is dropped until a new highest key is played.

Activate the Cantus Firmus with the CF-piston.



It is advisable not to use the Cantus Firmus in combination with the coupler III-II because this overrules the solo function of the Cantus Firmus.

### Transposer (TRANS.):

The Transposer function shifts the pitch by half-tone increments (from -8 to +8). The transposer setting can be read on the display (Trans: ...).

1. Press the TRANS.-piston.
2. Use the - and + pistons to set the pitch.
3. When the transposer change needs to be saved, press the ENTER-piston in the time the TRANS. piston is lit.

Utrecht, Bätz	
Location Organ Console	
Mem : 1	
Trans : -1	
Tune : 406,8Hz	
Temp : Original	
Cresc : Off	I/II/Pd III

### Cancel function (0):

Pressing the 0-piston cancels all registrations.

## 4.8 Pre-programmed memory locations

Pre-programmed memory locations are available by operating pistons PP to T and PL. These seven memory locations have factory settings (presets) appropriate for the quiet pianissimo to the loud tutti and the classical plenum. These pre-programmed memory locations are for each sample set.

### Calling up a pre-programmed memory location:

Press a pre-programmed memory location (PP-T or PL).

### Programming a pre-programmed memory location:



The current setting of the pre-programmed memory location will be lost.




Although it is possible to store any registration under a piston of a pre-programmed memory location it is advisable to select a registration matching the text of the piston.

1. Press the HR-piston.
2. Select the desired stops.
3. Press the SET-piston. Hold down this piston (to enable the storage function)
4. Press the desired pre-programmed memory location (PP-T or PL)
5. Release the SET-piston

---

## 4.9 Capture memory

Through use of the capture memory, a registration can be activated with just one piston. The capture memory consists of 50 levels (for ORGAN 1 – 5 = 250 levels). These levels can be seen on the display (Mem : ...). Each level has eight memory locations (pistons 1-8). The 400 capture memory locations are not pre-programmed and can be programmed by the musician. The capture memory locations are per sample set. Thus, the total amount of free programmable capture memory places in the LiVE III BDO is (400 locations times 5 Sample banks, equals) 2000.

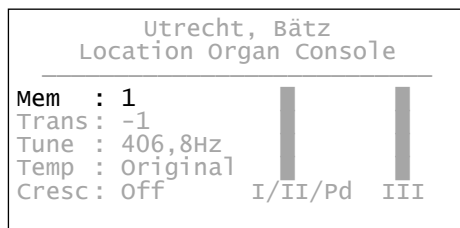

### Programming a capture memory location:



The current setting of the capture memory location will be lost.

1. Press the HR-piston.
2. Select the desired stops.
3. Use the - and + pistons to select a level (1-50) on the display.
4. Press the SET-piston. Hold down this piston (to enable the storage function)
5. Press the desired memory location (1-8).
6. Release the SET-piston.

### Calling up a capture memory location:

1. Use the - and + pistons to select the desired level (1-50) on the display.
2. Press the desired memory location (1-8).



Through use of the SEQ- and SEQ+ pistons previous or next memory locations (1–8) can be selected in steps of one. The lighted memory location piston (1–8) and the memory level shown in the display indicate the selected location.


## 4.10 Crescendo pedal

The crescendo pedal can be used to activate 20 registrations step-by-step. These registrations start with very quiet (pianissimo) to very loud (tutti). The default registrations of the 20 steps can be changed. See §5.5.1 Crescendo.


---

### Activating the crescendo pedal

If the crescendo pedal is not activated it is indicated on the displays with `Cresc:Off`.

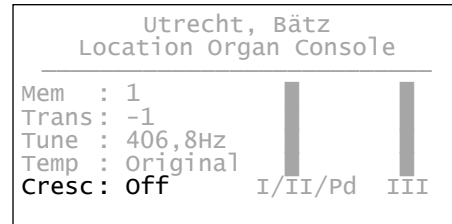

Use the CR-piston to activate the crescendo pedal. The display indicates the current step.

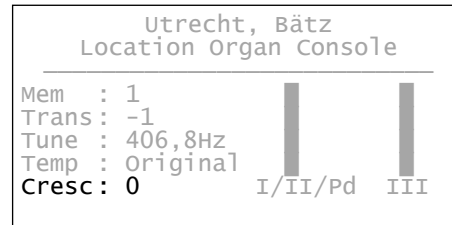

### Crescendo pedal as additional swell pedal

The crescendo pedal can also be configured as a swell pedal see §5.6.3 Expression Pedals. If the crescendo pedal is set as additional swell pedal, all functions of the original crescendo pedal are deactivated.

## 4.11 Quick Access

Quick Access is a function to quickly access certain functions of the organ.

### 4.11.1 Programming mode crescendo pedal



This function is not available if no expression pedal is set as crescendo pedal.

Pressing the ENTER-and CR-piston simultaneously enters the programming mode of the crescendo pedal. See §5.5.1 Crescendo, sub 6 for next steps.



---

## 5 JOHANNUS MENU

In the Johannus Menu several functions of the organ can be set:

- Press the MENU piston to activate the Johannus Menu on the display.
- Navigate in the menu with the - and + pistons.
- Confirm a choice by pressing the ENTER-piston.
- Cancel or step back in the menu by pressing the MENU-piston.

The Johannus Menu consists of the following functions:

Function	More information
<b>Reverb Volume</b>	§ 5.1
<b>Fine Tune</b>	§ 5.2
<b>Temperaments</b>	§ 5.3
<b>Upload Organ</b>	§ 5.4
<b>Organ Settings</b>	§ 5.5
➤ Crescendo	
➤ Datadump	
➤ Expression Pedals	
➤ Intonation	
➤ Key Volumes	
➤ MIDI Config	
➤ Reset	
➤ Sample Set Version	
<b>System Settings</b>	§ 5.6
➤ Aux In Level	
➤ Default Ambiance	
➤ Default Organ	
➤ Headphones/Aux Out	
➤ Keyboard Mode	
➤ Reset	
➤ Rear Speakers*	
➤ Side Speaker Level	
➤ Stop Numbers	
➤ Tone Control	
➤ Version	

Note: Rear Speaker is optional

### 5.1 Reverb Volume

With the function Reverb Volume you can set the volume of the reverb from 0 - 100%.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Reverb Volume` function on the display.
3. Press the ENTER-piston. The current reverb volume appears on the display behind `Level: .`
4. Use the - and + pistons to select the desired level.
5. Press the ENTER-piston to confirm.
6. Press the MENU-piston to exit the Johannus Menu.

---

## 5.2 Fine Tune

The Fine Tune function shifts the pitch in steps of 1 cent, from -50 till +50 cents. The frequency adapts automatically. The set pitch can always be read on the display behind `Tune :`.

```
Fine Tune:
0 cents

Frequency: 431.0 Hz
Use -/+, ENTER or MENU
```

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Fine Tune` function on the display.
3. Press the ENTER-piston. The Fine Tune setting appears in cents on the display.
4. Use the - and + pistons to select the desired pitch.
5. Press the ENTER-piston to program the new setting and to return to the Johannus Menu.
6. Press the MENU-piston to exit the Johannus Menu. The actual Fine Tune setting appears in cents on the display behind the current transposer setting (`Trans: ../..c`).

## 5.3 Temperaments

The Temperaments function sets the temperament. The set temperament can be read on the display behind the `Temp :` text.

There are twelve different temperaments:

- Original (original temperament)
- Equal (normal temperament)
- Young II
- Vallotti
- Kirnberger III
- Kirnberger II
- Neidhardt III
- Werckmeister III
- 1/6 Meantone (1/6 comma meantone)
- 1/5 Meantone (1/5 comma meantone)
- 1/4 Meantone (1/4 comma meantone)
- Pythagorean

Besides these twelve temperaments it is possible to configure a custom temperament:

- Custom (free programmable temperament)

### Selecting a temperament

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Temperaments` function on the display.
3. Press the ENTER-piston. A list of available temperaments appears on the display. The pointer indicates the current temperament.
4. Use the - and + pistons to select the desired temperament.

5. Press the ENTER-piston to program the new setting and to return to the Johannes Menu.
6. Press the MENU piston twice to exit the Johannes Menu.

### Programming a custom temperament

With function Custom Prog. it is possible to create a personal temperament. Every key can be detuned with increments of 1 cent. The minimum value is -32 cents; the maximum value is +32 cents.



The programming can be done using the *middle octave of Manual II* and is automatically calculated for all keys of the organ.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Temperaments` function on the display.
3. Press the ENTER-piston. A list of available temperaments appears on the display. The pointer indicates the current temperament.
4. Use the - and + pistons to select the `Custom Programming` function.
5. Press the ENTER-piston.
6. Press and hold a key of the middle octave of Manual I. The detune setting of the pressed key appears on the display. The given detuning is compared to the equal temperament.
7. Use the - and + pistons to select the desired pitch of the pressed key.
8. If necessary repeat steps 6 and 7 for another key of the middle octave.
9. Press the MENU piston three times to exit the Johannes Menu.



Using the reset procedure `Cust. Temperament def.` the Custom Temperament can be reset to equal temperament. See § 5.5.8 Reset.

## 5.4 Upload Organ

With the function Upload Organ you can load sample sets (recordings of pipe organs) from a prepared USB stick, into the Johannes LiVE's memory bank. The major advantage of storing a full recording is that you can switch effortlessly between your selected pipe organs, with pistons ORGAN 1 - 5.

```
Upload Organ:
> 1: Cavaillé-Coll, Paris
  2: Utrecht, Bätz
  3: Empty
  4: Empty
  5: Empty
```

Use -/+, ENTER or MENU

If you've saved more than five sample sets to organ memory, you can easily reload a new one from USB by overwriting one of the existing sample sets. If you want to return to your original selection, simply reload the sample set you overwritten into memory.

1. Insert the (prepared) USB stick, with sample set(s), in the USB port of the organ. Use USB sticks with storage space between 4 GB and 32 GB, (pre) formatted with FAT32 file system. Note that other file format systems, such as "NTFS", or "ExFAT" will not work. Recommended is to use the USB key as delivered with the organ, or which you ordered later.
2. Press the MENU-piston.

3. Use the – and + pistons to select the function `Upload Organ` on the display.
4. Press the ENTER-piston. Five options appear on the display. The pointer indicates the current choice. These five numbers correspond with the ORGAN 1 till ORGAN 5-pistons.
5. Use the – and + pistons to select the desired memory slot location:
  - Select the option `Empty` if you desire to copy the sample set to an empty location.
  - Select an option where a sample set has already been stored, if you would like to overwrite this with a new sample set. – The existing intonation data will be lost, insofar as it deviates from the factory settings. To secure this intonation data, see § 5.5.4 “Intonation”.
6. Press the ENTER-piston to confirm. A message will appear on the screen that an USB stick is being searched. Please wait.
7. A message appears on the display that the sample set is being uploaded. This can take 15-20 minutes. Do not turn off the organ in the meanwhile.
8. As soon as the upload is 100% , you will automatically return to the main screen. You can play the new sample set of the pipe organ directly.

## 5.5 Organ Settings

With the Organ Settings menu you can change the settings per sample set, in memory banks, with pistons “ORGAN 1 – 5”. The Organ Settings menu consists of the following sub-functions:

- Crescendo § 5.5.1
- Datadump § 5.5.2
- Expression Pedals § 5.5.3
- Intonation § 5.5.4
- Key Volumes § 5.5.5
- MIDI Config § 5.5.6
- Reset § 5.5.7
- Sample Set Version § 5.5.8

### 5.5.1 Crescendo

The crescendo pedal contains 20 pre-programmed registrations. These registrations start with very quiet (pianissimo) to very loud (tutti). These pre-programmed registrations can be changed.



Step 0 of the crescendo pedal cannot be changed.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available Organ Settings appears on the display.
4. Use the - and + pistons to select the `Crescendo` function on the display.
5. Press the ENTER-piston. The first step of the crescendo pedal appears on the display.
6. Use the - and + pistons to select the step which has to be changed.

7. Change the registration and press the ENTER-piston to save the new registration in the memory of the organ.
8. Repeat steps 6 and 7 if more crescendo pedal steps has to be changed.
9. Press the MENU piston three times to exit the Johannus Menu.

### 5.5.2 Datadump

The Datadump function saves several settings from the organ to an USB stick. This requires a USB stick, with a size of up to 32 GB and pre-formatted with the FAT32 file system.

The settings that are saved are: the contents of all capture memory locations and all settings that can be set via the Johannus Menu, except Key Volumes. Key Volume settings are a part of the intonation data and can be received with the optional Johannus Intonat 7 software.

#### a. Saving data from the organ

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available Organ Settings appears on the display.
4. Use the - and + pistons to select the `Datadump` function on the display.
5. Press the ENTER-piston. The Datadump menu appears on the display.
6. Use the - and + pistons to select the `Save datadump` function.
7. Make sure the desired USB stick, up to a maximum storage size of 32 GB, is correctly connected and is pre-formatted with the **FAT32 file system**.
8. Press the ENTER-piston. When data is being sent, `Busy...` appears on the display.



It is possible that there is already a file present. You will be asked whether the file should be overwritten. Use the - and + pistons to select the function, then press the ENTER-piston to confirm.



Do not use the organ when the `Busy...` text is on the display.

9. If the data dump is complete, the Datadump menu appears on the display.
10. Press the MENU-piston three times to exit the Johannus Menu.

#### b. Uploading data to the organ



Make sure to upload only data files which are created with the same instrument. Uploading a data file from another instrument may jeopardize the functioning of your instrument.

1. Follow the steps 1 to 5 as described above at **a. Saving data from the organ**.
2. Use the - and + pistons to select the `Load datadump` function.
3. Make sure the desired USB-stick is inserted properly.

4. Press the ENTER-piston. When data is being sent, `Busy...` appears on the display.
5. After the text `Uploading successful` and `Reboot the organ` turn the organ off and on again.

### 5.5.3 Expression Pedals

The organ is equipped with PEPC™ (Programmable Expression Pedal Configuration). This function makes it possible to configure each expression pedal to one's own discretion.

We distinguish two types of expression pedals:

**Swell pedal:** dynamics by increase or decrease of volume. In a pipe organ this is achieved by closing or opening the swell shutters of a swell box. See also § 4.2 Expression pedal.

**Crescendo pedal:** dynamics by increasing or decreasing the amount of stops. See also § 4.10 Crescendo Pedal.



- a. An expression pedal can be configured for several divisions at the same time.
- b. A division can only be connected to one expression pedal at the same time.
- c. An expression pedal cannot be configured as an expression pedal and a crescendo pedal at the same time.

1. Press the MENU-piston.
2. Use the – and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available Organ Settings appears on the display.
4. Use the - and + pistons to select the `Expression Pedals` function on the display.
5. Press the ENTER-piston. The available expression pedals appear on the display.
6. Use the - and + pistons to select the expression pedal of which the function must be changed.
7. Press the ENTER-piston. The available possibilities appear on the display. Behind the possibilities the current setting is marked with a 'V'.
8. Use the - and + pistons to select the desired setting.
  - I: Expression pedal for Manual I
  - II: Expression pedal for Manual II
  - III: Expression pedal for Manual III
  - Cresc: Crescendo Pedal
9. Press the ENTER-piston. The pointer jumps to the chosen position.
10. Use the - and + pistons to select the functionality.
11. Press the ENTER-piston for confirmation.
12. Press the MENU piston to return to the Expression Pedals menu.
13. If necessary, repeat steps 6 to 12 for another expression pedal.
14. Press the MENU piston three times to exit the Johannus Menu.

---

#### 5.5.4 Intonation

The Intonation function saves voice settings from the organ to an USB stick. This requires a USB stick, with a storage size up to a maximum of 32 GB and pre-formatted with the FAT32 file system.

##### a. Saving Intonation data from the organ

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available Organ Settings appears on the display.
4. Use the - and + pistons to select the `Intonation` function on the display.
5. Press the ENTER-piston. The Intonation menu appears on the display.
6. Use the - and + pistons to select the `Save voicing` function.
7. Make sure the desired USB-stick, is inserted properly. It is recommended to save the intonation data with written description (on the stick itself):
  - to a separate USB-stick, with description of the sample set & version, or
  - to save the data to the same original sample set stick that it belongs to. –This will then be placed on the USB stick as a second intonation file, next to the factory intonation data.
8. Press the ENTER-piston. When data is being sent, `Busy...` appears on the display.



It is possible that there is already a file present. You will be asked whether or not the file should be overwritten. Use the - and + pistons to select the function, then press the ENTER-piston to confirm.



Do not use the organ when the `Busy...` text is on the display.

9. If the data dump is complete, the Intonation menu appears on the display. Note: Repeat (steps 5 – 9) for each ORGAN 1 – 5, if necessary.
10. Press the MENU-piston three times to exit the Johannus Menu.

##### b. Uploading intonation data to the organ



Make sure to upload only data files which are created with the same instrument. Uploading a data file from another instrument may jeopardize the functioning of your instrument.

1. Follow the steps 1 to 5 as above as described at **a. Saving data from the organ**.
2. Use the - and + pistons to select the `Load voicing` function.
3. Make sure the desired USB-stick, is inserted properly.
4. Press the ENTER-piston. When data is being sent, the message `Busy...` appears on the display.
5. If the data dump is complete, the Intonation menu appears on the display.
6. Press the MENU-piston three times to exit the Johannus Menu.

---

### 5.5.5 Key Volumes

The Key Volumes function makes it possible to adjust the key volumes of each stop. The Key Volumes function consists of the following sub-functions:

- a. Adjust
- b. Reset one stop
- c. Reset ALL stops

#### a. Adjust

The Adjust function sets the volume per key and per stop.

1. Switch off all stops.
2. Press the MENU-piston.
3. Use the - and + pistons to select the `Organ Settings` function on the display.
4. Press the ENTER-piston. A list with available Organ Settings appears on the display.
5. Use the - and + pistons to select the `Key Volumes` function on the display.
6. Press the ENTER-piston. The sub-functions of the Key Volumes menu appear on the display.
7. Use the - and + pistons to select the sub-function `Adjust` and press the ENTER-piston. A question to select a stop to adjust appears on the display.
8. Activate one stop. A question to press a key appears on the display.
9. Press one key on the corresponding division and hold the key. The display will now show following `Key`: the key indicator and following `Vol`: the volume.
10. Use the - and + pistons to set the desired volume.
11. Press the ENTER-piston to save the change. The message `Save changes?` appears on the display. Use the - and + pistons to select `No` or `Yes`.
12. Press the ENTER-piston to confirm.
13. If you have chosen `No`, you automatically return to the `Adjust` submenu. If you have chosen `Yes` the message `Programming Key Volume` appears on the display. After several seconds you will return to the `Key Volume` menu.
14. Press the MENU piston three times to exit the Johannus Menu.



More key volumes can be changed by pressing another key or by selecting another stop.

#### b. Reset one stop

The Reset one stop sub-function resets the key volumes for one stop to the factory setting.

1. Press the MENU-piston.
2. Switch off all stops.
3. Use the - and + pistons to select the `Organ Settings` function on the display.



- 
4. Press the ENTER-piston. A list with available Organ Settings appears on the display.
  5. Use the - and + pistons to select the `Key Volumes` function on the display.
  6. Press the ENTER-piston. The sub-functions of the Key Volumes menu appear on the display.
  7. Use the - and + pistons to select the `Reset one stop` sub-function on the display.
  8. Press the ENTER-piston. A question to select a stop to reset appears on the display.
  9. Activate one stop. A question to confirm appears on the display.
  10. Use the - and + pistons to select `No` or `Yes`.
  11. Press the ENTER-piston to confirm and to return to the Key Volumes menu.
  12. Press the MENU pistons three times to exit the Johannus Menu.

### **c. Reset ALL stops**

The Reset ALL stops function resets the key volumes of all stops to the factory setting.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available Organ Settings appears on the display.
4. Use the - and + pistons to select the `Key Volumes` function on the display.
5. Press the ENTER-piston. The sub-functions of the Key Volumes menu appear on the display.
6. Use the - and + pistons to select the `Reset ALL stops` sub-function on the display.
7. Press the ENTER-piston. A question to confirm appears on the display.
8. Use the - and + pistons to select `No` or `Yes`.
9. Press the ENTER-piston to confirm and to return to the Key Volumes menu.
10. Press the MENU-piston three times to exit the Johannus Menu.

### **5.5.6 MIDI Config**

MIDI is a protocol for communication between the organ and other devices, such as PC, Johannus MIDI Sequencer+ or other musical instruments.

The programmable MIDI stops allow you to control any module voice through any MIDI channel (1-16).

The four parts of the programmable MIDI code are: Channel, MSB, LSB and Voice.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available Organ Settings appears on the display.
4. Use the - and + pistons to select the `MIDI Config` function on the display.
5. Press the ENTER-piston. A question to select a MIDI stop to configure appears on the display.

- 
6. Activate the MIDI stop which has to be configured. The settings of the corresponding MIDI stop appear on the display. A pointer is located in front of the value of the MIDI channel.
  7. Use the - and + pistons to select the desired MIDI channel.
  8. Press the ENTER-piston. The pointer jumps to the MSB value.
  9. Use the - and + pistons to select the desired MSB value.
  10. Press the ENTER-piston. The pointer jumps to the LSB value.
  11. Use the - and + pistons to select the desired LSB value.
  12. Press the ENTER-piston. The pointer jumps to the Voice value.
  13. Use the - and + pistons to select the desired Voice value.
  14. Press the ENTER-piston. The selected configuration is now stored in memory. The pointer jumps back to the MIDI channel location.
  15. Press the MENU piston three times to exit the Johannus Menu.

### 5.5.7 Reset

The Reset function can be used to reset a number of setting per sample set to the factory settings.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available Organ Settings appears on the display.
4. Use the - and + pistons to select the `Reset` function on the display.
5. Press the ENTER-piston. The available Reset functions appear on the display.
6. Use the - and + pistons to select the desired reset procedure:
 

<code>Crescendo default:</code>	Resets to factory settings of the 20 steps of the crescendo pedal.
<code>Cust. Temperament def.:</code>	Resets the custom programmable temperament to equal temperament.
<code>Expression Pedals def.:</code>	Resets to factory settings of the expression pedals.
<code>Intonation default:</code>	Resets to factory settings of the intonation.
<code>Memory default:</code>	Clears the entire capture memory.
<code>MIDI default:</code>	Resets to factory settings of the MIDI stops.
<code>Preset default:</code>	Resets to factory settings of the pre programmed memory locations.
7. Press the ENTER-piston. A question to confirm appears on the display.
8. Use the - and + pistons to select `No` or `Yes`. Press the ENTER-piston to confirm and to return to the Reset menu.
9. Press the MENU piston three times to exit the Johannus Menu.

---

### 5.5.8 Sample Set Version

The Sample Set Version function shows the date of the sample set of the activated organ bank.

1. Press the MENU piston.
2. Use the - and + pistons to select the `Organ Settings` function on the display.
3. Press the ENTER-piston. A list with available `Organ Settings` appears on the display.
4. Use the - and + pistons to select the `Sample Set Version` function on the display.
5. Press the ENTER-piston. The data of the sample set that is currently loaded in the organ appears on the display.
6. Press the MENU piston three times to exit the Johannus Menu.

Sample Set Version:  
Utrecht, Bätz  
Version 1.0

Use ENTER or MENU

## 5.6 System Settings

With the System Settings menu you can change the settings for the entire LiVE III organ. The System Settings menu consists of the following sub-functions:

- Aux In Level § 5.6.1
- Default Ambiance § 5.6.2
- Default Organ § 5.6.3
- Headphones / Aux Out § 5.6.4
- Keyboard Mode § 5.6.5
- Reset § 5.6.6
- Rear Speaker level § 5.6.7
- Side Speakers Level § 5.6.8
- Stop Numbers § 5.6.9
- Tone Control § 5.6.10
- Version § 5.6.11

### 5.6.1 Aux In Level

The System Setting 'Aux In Level' function sets the Auxiliary Input Level at the desired level at the startup of the organ. When the Auxiliary input is not in use, the preferred setting is 0%. Older models may not have this 'Aux In Level' function.

1. Press the MENU-piston
2. Use the – and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available System Settings appears on the display.
4. Use the – and + pistons to select the `Aux In Level` setting.
5. Press the ENTER-piston.
6. Use the – and + pistons to select the desired Auxiliary input level.
7. Press the ENTER-piston to confirm and to return to the System Settings menu.
8. Press the MENU-piston twice to exit the Johannus Menu.

---

### 5.6.2 Default Ambiance

The System Setting Default Ambiance determines which listening position is selected at the startup of the organ.

1. Press the MENU-piston
2. Use the – and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available System Settings appears on the display.
4. Use the – and + pistons to select the `Default Ambiance` setting.
5. Press the ENTER-piston. A list with available listening positions appears on the display with a pointer for the selected listening position.
6. Use the – and + pistons to select the desired listening position.
7. Press the ENTER-piston to confirm and to return to the System Settings menu.
8. Press the MENU-piston twice to exit the Johannus Menu.

### 5.6.3 Default Organ

The System Setting Default Organ determines which sample set is selected at the startup of the organ.

1. Press the MENU-piston
2. Use the – and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available System Settings appears on the display.
4. Use the – and + pistons to select the `Default Organ` setting.
5. Press the ENTER-piston. A list with available sample sets appears on the display with a pointer for the selected sample set.
6. Use the – and + pistons to select the desired sample set.
7. Press the ENTER-piston to confirm and to return to the System Settings menu.
8. Press the MENU-piston twice to exit the Johannus Menu.

### 5.6.4 Headphones / Aux Out

System Setting Headphones / Aux Out determines the volume level of the headphones / Aux-output at startup of the organ.

1. Press the MENU piston.
2. Use the - and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available system settings appears on the display.
4. Use the - and + pistons to select the `Headphones / Aux Out` function.
5. Press the ENTER-piston. The current setting appears on the display.
6. Use the - and + pistons to select the desired level.

- 
7. Press the ENTER-piston to confirm and to return to the System Settings menu.
  8. Press the MENU piston twice to exit the Johannus Menu.

### 5.6.5 Keyboard Mode

The Keyboard Mode function sets the operation of the keys.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available system settings appears on the display.
4. Use the - and + pistons to select the `Keyboard Mode` function on the display.
5. Press the ENTER-piston. The available manuals appear on the display.
6. Use the - and + pistons to select the manual of which you would like to change the setting.
  - I: Manual I
  - II: Manual II
  - III: Manual III
7. Press the ENTER-piston. The available options appear on the display, with a pointer for the selected setting.
8. Use the - and + pistons to select a setting for the operation of the keys.
  - `Automatic`: The manual has been set to High. When activating a programmable MIDI, the manual will be set to Velocity automatically.
  - `High`: The keys respond when touched very lightly.
  - `Low`: The keys respond when pressed further.
  - `Velocity`: The keys are touch-sensitive. For organ stops this means that the setting for 'low' is being used.
9. Press the ENTER-piston to program the settings. The available manuals appear on the display again.
10. Repeat steps 6 to 9 to change the setting of another manual or press the MENU piston three times to exit the Johannus Menu.

### 5.6.6 Reset

The Reset function can be used to reset a setting to the factory setting.

1. Press the MENU-piston.
2. Use the - and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available system settings appears on the display.
4. Use the - and + pistons to select the `Reset` function on the display.
5. Press the ENTER-piston. The available Reset functions appear on the display.
6. Use the - and + pistons to select the desired reset procedure:
  - `Keyboard Mode default`: Resets to factory settings of the keys.
7. Press the ENTER-piston. A question to confirm appears on the display.
8. Use the - and + pistons to select `No` or `Yes`. Press the ENTER-piston to confirm and to return to the Reset menu.
9. Press the MENU piston three times to exit the Johannus Menu.

---

### 5.6.7 Rear Speakers (optional)

Optional: The System Settings function Rear Speakers determines the volume level (On / Off) of the external Rear Surround Loudspeakers at startup of the organ display.

1. Press the MENU piston.
2. Use the - and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available System Settings appears on the display.
4. Use the - and + pistons to select the `Rear Speakers` function on the display.
5. Press the ENTER-piston. The current settings for the Rear Speakers appear on the display.
6. Use the - and the + pistons to select the function.



When Rear Speakers are not used, or not connected, the best sound quality can be obtained by `Rear Speakers 0% (Off)`.



Do not connect, do not use internal connections for external speakers by yourself. Refer all servicing to your retailer, or Global Organ Group B.V.

7. Press the ENTER-piston. The pointer jumps to the set level.
8. Use the - and + pistons to select the desired selection.
9. Press the ENTER-piston to confirm and to return to the Rear Speakers menu.
10. Press the MENU piston three times to exit the Johannus Menu.

### 5.6.8 Side Speakers Level

The System Settings function Side Speakers Level determines the volume level of the Surround Loudspeakers at startup of the organ.

1. Press the MENU piston.
2. Use the - and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available System Settings appears on the display.
4. Use the - and + pistons to select the `Side Speakers Level` function on the display.
5. Press the ENTER-piston. The current settings for the left and the right side speaker appear on the display.
6. Use the - and + pistons to select the side of which the level has to be changed.
7. Press the ENTER-piston. The pointer jumps to the set level.
8. Use the - and + pistons to select the desired level (0-100%).
9. Press the ENTER-piston to confirm and to return to the Side Speakers Level menu.



For a proper balance of the Surround sound it is advisable to keep both sides on an equal level. Use only unequal levels to correct different volumes caused by, for example, reflective surfaces on one side of the organ.

10. Press the MENU piston three times to exit the Johannus Menu.

---

### 5.6.9 Stop Numbers

This System Settings function 'Stop Numbers' determines if the Stop Numbers will be updated automatically on the a small dynamic displays, when a sampleset is selected with sample bank pistons (Organ 1 - 5). The appropriate stoplist names of the selected organ (1 – 5) will be visible on the small dynamic displays above each stop individually, see also 4.5.1.

When desired, it is possible to change the individual register stop position. These can be exchanged / swapped (together with the correct stop list names), using Johannus Intonat software.

### 5.6.10 Tone Control

The function Tone Control allows you to set the bass and brilliance of the organ in steps of 0,5 decibel from -6 dB to +6 dB. The bass and brilliance level appear on the display.

1. Press the MENU piston.
2. Use the - and + pistons to select the System Settings function on the display.
3. Press the ENTER-piston. A list with available System Settings appears on the display.
4. Use the - and + pistons to select the Tone Control function on the display.
5. Press the ENTER-piston. The current settings for the Bass and Brilliance speaker appear on the display. Use the - and + pistons to select the function that has to be changed.  
Bass:                    behind it is the current bass level.  
Brilliance:            behind it is the current brilliance level.
6. Use the - and + pistons to select the function of which the level has to be changed.
7. Press the ENTER-piston. The pointer jumps to the set level.
8. Use the - and + pistons to select the desired level (-6 dB to + 6dB)
9. Press the ENTER-piston to confirm and to return to the Tone Control menu.
10. Repeat steps 6 to 9 to change the setting of function.
11. Press the MENU piston three times to exit the Johannus Menu.

```
Tone Control:
> Bass:    0,0 dB
  Brilliance:    0,0 dB

Use -/+, ENTER or MENU
```

### 5.6.11 Version

The Version function shows the model type, software version number, as well as the organ's order number. In this menu you can also upload a new firmware version from an USB stick.

#### a. Actual version

1. Press the MENU piston.
2. Use the - and + pistons to select the System Settings function on the display.

```
Actual version:
LiVE III
V3.35
Hw GOG:V3, HP amps
Reverb 2.0.1
Order number: 45689

Use ENTER or MENU
```

- 
3. Press the ENTER-piston. A list with available System Settings appears on the display.
  4. Use the - and + pistons to select the `Version` function on the display.
  5. Press the ENTER-piston. The Version menu appears on the display.
  6. Use the - and + pistons to select the `Actual version` function on the display.
  7. Press the ENTER-piston. The data of the software of the organ appears on the display.
  8. Press the MENU piston four times to exit the Johannus Menu.

#### **b. Load new version**



Make sure to upload only data files which are created with the same instrument. Uploading a data file from another instrument may jeopardize the functioning of your instrument.

1. Press the MENU piston.
2. Use the - and + pistons to select the `System Settings` function on the display.
3. Press the ENTER-piston. A list with available System Settings appears on the display.
4. Use the - and + pistons to select the `Version` function on the display.
5. Press the ENTER-piston. The Version menu appears on the display.
6. Use the - and + pistons to select the `Update organ` function on the display.
7. Make sure the desired USB-stick, is inserted properly.
8. Press the ENTER-piston. On the display appears the question whether the current version may be overwritten by another.
9. Use the - and + pistons to select `No` or `Yes`.
10. Press the ENTER-piston. When data is being sent, `Busy...` appears on the display.
11. When the update is complete, the organ will reboot.



---

## 6 MAINTENANCE, TROUBLESHOOTING AND WARRANTY

### 6.1 Maintenance

#### Overview

Component	Maintenance	Frequency
Cabinet	Cleaning. See § 6.1.1	As required
Manuals	Cleaning and removing scratches. See § 6.1.2	As required

#### 6.1.1 Maintenance of the cabinet



Do not use furniture polish or teak oil to clean the organ cabinet.  
Direct sunlight may discolor the organ cabinet.

1. Clean the cabinet with a damp cloth.
2. Rub the cabinet dry with a lint-free cloth.

#### 6.1.2 Maintenance of the manuals

By default, the Johannes LIVE III comes with Synthetic keyboards with a wooden core.



Do not use aggressive cleaning agents such as paint thinner or acetone to remove dirt.

1. Clean the manuals with a damp cloth.
2. Rub the manuals dry with a lint-free cloth.
3. Remove any scratches with car polish.

### 6.2 Problems

#### Overview

Symptom	Cause	Solution
Pedal board does not work properly	The pedal magnet is making poor contact with the magnetic switch at the rear of the pedal front cover.	Reposition the pedal board. See § 2.1.2.
Organ functions do not work properly	The organ is not grounded.	Connect the organ to a grounded power socket.
Display message: Error: Usb code 3	USB stick contains stored file data on a format (such as exFAT, or NTFS), other than the required <b>FAT32 file system</b> and/or has a storage size greater than 32GB.	Store data on a pre-formatted USB stick with the <b>FAT32 file system</b> , 32GB or smaller size.

### 6.3 Warranty

The conditions are specified in the warranty certificate. The warranty is void if changes or repairs are made to the organ by persons or organizations that are not authorized by Global Organ Group B.V.

## 7 SPECIFICATIONS

### 7.1 MIDI Implementation Chart

JOHANNUS Organs

MIDI Implementation card

Date: October 2015  
Version 1.00

Functions		Transmitted	Recognized	Remarks
<b>Basic Channel</b>	Default Changes	See MIDI Specs See MIDI Specs	See MIDI Specs Y <sup>1</sup>	See MIDI Specs
<b>Mode</b>	Default Messages Altered	Mode 3 N * * * * *	Mode 3 N N	
<b>Note Number</b>	True Voice	36 - 96 * * * * *		
<b>Velocity</b>	Note ON Note OFF	9nH v=1 - 127 9nH (v=64) 9nH (v=0)	9nH v=1 - 127 9nH v=1 - 127 9nH v=0, 8nH v=*	Velocity ON Velocity OFF *=irrelevant
<b>After Touch</b>	Keys Channels	N N		
<b>Fine Tune Bend</b>		N		
<b>Control Change</b>	7 11 100/101/6/38 100/101/6	Y Y Y Y		General Volume Expr. pedals Fine Tune Transposer
<b>Program Change</b>	: True#	See MIDI Specs * * * * *	See MIDI Specs See MIDI Specs	See MIDI Specs See MIDI Specs
<b>System Exclusive</b>		See MIDI Specs	See MIDI Specs	See MIDI Specs
<b>Common</b>	: Song Pos : Song Sel : Tune	N N N	N N N	
<b>System Real Time</b>	: Clock : Commands	N N	N N	
<b>Aux</b>	: Reset All Contr. : Local ON/OFF : All Notes OFF : Active Sense : Reset	N N Y N N	N N Y N N	
<b>Notes</b>	<sup>1</sup> Depends on number of divisions			

Mode 1: OMNI ON, POLY  
Mode 3: OMNI OFF, POLY

Mode 2: OMNI ON, MONO  
Mode 4: OMNI OFF, MONO

Y=YES  
N=NO

---

## 7.2 MIDI Specifications

This paragraph describes the specifications on the MIDI Implementation Chart in more detail.

### Default basic channels (transmitted/recognized)

7:	Pedal
8:	Manual I
9:	Manual II
10:	Manual III
16:	Accessories

### Basic channel changes (transmitted)

Can be programmed through the MIDI Config. See § 5.5.5 MIDI Config.

### Control changes (transmitted)

- Controller 7 (07h) General volume, with volume values 40 (28h) – 127 (7Fh).
- Controller 11 (0Bh) Swell pedal, with volume values 55 (37h) – 127 (7Fh).
- Controller 6 (06h) Fine Tune, with Fine Tune values 33 (21h) - 95 (5Fh).  
Fine Tune value 64 (40h) = A = 0 cents.  
The following applies to the Fine Tune:  
LSB 100 (64h) 1 (01h) and the MSB 101 (65h) 0(00h).  
Transposer, with transposer values 56 (38h) - 72 (48h).  
Transposer value 64 (40h) = A = center.  
The following applies to the transposer:  
LSB 100 (64h) 2 (02H) and the MSB 101 (65h) 0(00h).

### Control changes (recognized)

- Controller 7 (07h) General volume, with volume values 0 (00h) – 127 (7Fh). Volume values less than 40 (28h) are treated as 40 (28h).
- Controller 11 (0Bh) Swell pedal, with volume values 0 (00h) – 127 (7Fh). Volume values less than 55 (37h) are treated as 55 (37h).

### Program changes (transmitted/recognized)

Organ stops: Depends on the number of stops and the sequence of stops.

MIDI stops (programmable): 1-128. See § 5.5.5 MIDI Config.

### System exclusive messages (transmitted/recognized)

Each 'sys ex' (system exclusive) message largely looks the same. The first 7 bytes and the last byte are always the same. Only the value of the 8th byte varies. This is the 'sys ex message' that Johannus generally uses: F0 00 4A 4F 48 41 53 XX F7 (hexadecimal). The 'sys ex messages' described below only indicates the value of the 8th byte (XX) and the output from which it is transmitted.

---

**All stops off**

The 'all stops off' sys ex code is 7F. This sys ex code is transmitted through the MIDI SEQ. output when the 0 piston is pressed for a longer time. When an 'all stops off' sys ex code is received, all stops on the instrument are switched off.

**Pushbutton values**

When a piston is pressed, a sys ex code is transmitted with the value of the piston that is pressed (for example PP = 00 P = 01) through the MIDI MOD. output. These sys ex codes are only important when the Johannus sound module CSM 128 is connected to your instrument.

**Other MIDI codes (transmitted)**

Press the 0 piston to transmit the sys ex code, 'all stops off' and all volume settings through the MIDI SEQ. output.

## 7.3 Specifications of Instrument

This paragraph describes the specifications of the instrument.

Items for instrument type:		LIVE III BDO
<b>Keyboards, stops, etc.</b>	Swell shoes	2 wooden swell shoes
	Manuals	3 x 61 keys Synthetic keyboards with wooden core. optional: 3 x 61 keys - wooden keyboards (ebony/oak) with wooden core
	Stops	50 assignable stops; drawknobs with wooden stem, optional: knobs with LED indication.
	Stop jambs	Straight stop jambs
	Pedalboard (options)	30-NOTE STRAIGHT PEDAL BOARD 30-NOTE CONCAVE PEDAL BOARD 30-NOTE RACO PEDAL BOARD
<b>8.1 Audio System Internal speakers</b>	Subwoofer	1
	Fullrange driver	8
<b>External rear speaker connections (option)</b>	External rear speaker connections (optional)*	Optional 2 external rear speaker connections, for reverb sound from behind*. Note: Speaker impedance 4-8 Ohms. The 2 speakers are not included.
<b>Connectors</b>	Phones jack	6.3 mm (Stereo)
	Output jack	6.3 mm (2x mono AUX OUT)
	Input jack	6.3 mm (2x mono AUX IN)
	MIDI connectors	3 (In, MOD, SEQ)
	USB port	1 (Memory port for USB Stick; up to 32 GB, FAT32 pre-formatted)
	Fixed AC cable with connector	1
<b>Music rack</b>	Integrated music rack	1
<b>Power consumption</b>		190 W, 80 W idle Mode
<b>Operational Ambient Temperature Range</b>		32-113 °F; 0-45 °C.
<b>Mains Supply Voltage</b>		This instrument is adjusted to a mains supply voltage of: 220V, 230V & 240V 50/60Hz, or 100, 120V & 240V 50/60Hz. Before connecting the instrument, check if your mains voltage corresponds to the voltage indicated on the serial plate (see bottom below keyboards).
<b>Console Dimensions</b>	Height	180 cm
	Width	160 cm
	Depth	65 cm
	Depth with Pedalboard	103 cm
<b>Weights</b>	Console	225 kg
	Bench	20 kg (or option: Adjustable bench, 27 kg)
	Pedalboard	22 kg
	Total Weight	274 kg

Specification v.2.00: In the interest of product improvement, the specifications and/or appearance of this Organ are subject to change without prior notice. Please note that the actual dimensions and weight may differ slightly from this specification due to the woodwork and (internal) options. The above described dimensions (and shape) of the LIVE III model differ from previous model, before November 2019.

When optional Rear Speaker connections are not used, the best sound quality can be obtained by setting to 0% (Off) in the menu 'System Settings', 'Rear Speakers'.

For the USA: This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC rules as documented for identified product above. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications.

However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause interference to radio or television reception, which can be determined by turning the equipment o- and then on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

This equipment referenced in this declaration is identical to the Organ tested and found acceptable with the standards. The technical records maintained by the responsible party continue to reflect the equipment being produced under this Declaration of Conformity within the variation that can be expected due to quantity production and testing on a statistical basis.

This equipment requires shielded interface cables in order to meet FCC class B limit. Any unauthorized changes or modifications not expressly approved by the party responsible for compliance could void the user authority to operate the equipment.

For Canada: **NOTICE.** This Class B digital apparatus meets all requirements of the Canadian Interference-Causing Equipment Regulations.

**AVIS.** *Cet appareil numérique de la classe B respecte toutes les exigences du Règlement sur le matériel brouilleur du Canada.*

For C.A. US (Proposition 65): **WARNING.** This product contains chemicals known to cause cancer, birth defects and other reproductive harm, including lead.

## For China:

# 有关产品中所含有害物质的说明

本资料就本公司产品中所含的特定有害物质及其安全性予以说明。

本资料适用于 2007 年 3 月 1 日以后本公司所制造的产品。

## 环保使用期限



此标志适用于在中国国内销售的电子信息产品，表示环保使用期限的年数。所谓环保使用期限是指在自制造日起的规定期限内，产品中所含的有害物质不致引起环境污染，不会对人身、财产造成严重的不良影响。环保使用期限仅在遵照产品使用说明书，正确使用产品的条件下才有效。不当的使用，将会导致有害物质泄漏的危险。

## 产品中有毒有害物质或元素的名称及含量

部件名称	有毒有害物质或元素					
	铅(Pb)	汞(Hg)	镉(Cd)	六价铬(Cr(VI))	多溴联苯(PBB)	多溴二苯醚(PBDE)
外壳(壳体)	×	○	○	○	○	○
电子部件(印刷电路板等)	×	○	×	○	○	○
附件(电源线、交流适配器等)	×	○	○	○	○	○

○：表示该有毒有害物质在该部件所有均质材料中的含量均在 SJ/T11363-2006 标准规定的限量要求以下。

×：表示该有毒有害物质至少在该部件的某一均质材料中的含量超出 SJ/T11363-2006 标准规定的限量要求。

因根据现有的技术水平，还没有什么物质能够代替它。

## For EU, UK:

### For EU Countries



**UK** This symbol indicates that in EU countries, this product must be collected separately from household waste, as defined in each region. Products bearing this symbol must not be discarded together with household waste.

**DE** Dieses Symbol bedeutet, dass dieses Produkt in EU-Ländern getrennt vom Hausmüll gesammelt werden muss gemäß den regionalen Bestimmungen. Mit diesem Symbol gekennzeichnete Produkte dürfen nicht zusammen mit den Hausmüll entsorgt werden.

**FR** Ce symbole indique que dans les pays de l'Union européenne, ce produit doit être collecté séparément des ordures ménagères selon les directives en vigueur dans chacun de ces pays. Les produits portant ce symbole ne doivent pas être mis au rebut avec les ordures ménagères.

**IT** Questo simbolo indica che nei paesi della Comunità europea questo prodotto deve essere smaltito separatamente dai normali rifiuti domestici, secondo la legislazione in vigore in ciascun paese. I prodotti che riportano questo simbolo non devono essere smaltiti insieme ai rifiuti domestici. Ai sensi dell'art. 13 del D.Lgs. 25 luglio 2005 n. 151.

**ES** Este símbolo indica que en los países de la Unión Europea este producto debe recogerse aparte de los residuos domésticos, tal como está regulado en cada zona. Los productos con este símbolo no se deben depositar con los residuos domésticos.

**PT** Este símbolo indica que nos países da UE, a recolha deste produto deverá ser feita separadamente do lixo doméstico, de acordo com os regulamentos de cada região. Os produtos que apresentem este símbolo não deverão ser eliminados juntamente com o lixo doméstico.

**NL** Dit symbool geeft aan dat in landen van de EU dit product gescheiden van huishoudelijk afval moet worden aangeboden, zoals bepaald per gemeente of regio. Producten die van dit symbool zijn voorzien, mogen niet samen met huishoudelijk afval worden verwijderd.

**DK** Dette symbol angiver, at i EU-lande skal dette produkt opsamlles adskilt fra husholdningsaffald, som defineret i hver enkelt region. Produkter med dette symbol må ikke smides ud sammen med husholdningsaffald.

**NO** Dette symbolet indikerer at produktet må behandles som spesialavfall i EU-land, iht. til retningslinjer for den enkelte regionen, og ikke kastes sammen med vanlig husholdningsavfall. Produkter som er merket med dette symbolet, må ikke kastes sammen med vanlig husholdningsavfall. Apparatet må tilkoples jordet stikkontakt.

**SE** Symbolen anger att i EU-länder måste den här produkten kasseras separat från hushållsavfall, i enlighet med varje regions bestämmelser. Produkter med den här symbolen får inte kasseras tillsammans med hushållsavfall. Apparaten skall anslutas till jordat uttag.

**FI** Tämä merkintä ilmaisee, että tuote on EU-maissa kerättävä erillään kotitalousjätteistä kunkin alueen voimassa olevien määräysten mukaisesti. Tällä merkinnällä varustettuja tuotteita ei saa hävittää kotitalousjätteen mukana. Laite on liitettävä suojakoskettimilla varustettuun pistorasiaan.

**HU** Ez a szimbólum azt jelenti, hogy az Európai Unióban ezt a terméket a háztartási hulladéktól elkülönítve, az adott régióban érvényes szabályozás szerint kell gyűjteni. Az ezzel a szimbóllummal ellátott termékeket nem szabad a háztartási hulladék közé dobni.

**PL** Symbol oznacza, że zgodnie z regulacjami w odpowiednim regionie, w krajach UE produktu nie należy wyrzucać z odpadami domowymi. Produktów opatrzonych tym symbolem nie można utylizować razem z odpadami domowymi.

**CZ** Tento symbol udává, že v zemích EU musí být tento výrobek sbírán odděleně od domácího odpadu, jak je určeno pro každý region. Výrobky nesoucí tento symbol se nesmí vyhazovat spolu s domácím odpadem.

**SK** Tento symbol vyjadruje, že v krajinách EÚ sa musí zber tohto produktu vykonávať oddelene od domového odpadu, podľa nariadení platných v konkrétnej krajine. Produkty s týmto symbolom sa nesmú vyhazovať spolu s domovým odpadom.

**EE** See sümbol näitab, et EL-i maades tuleb see toode olemprügisti eraldi koguda, nii nagu on igas piirkonnas määratletud. Selle sümboliga märgitud tooteid ei tohi ära visata koos olmeprügiga.

**LT** Šis simbolis rodo, kad ES šalyse šis produktas turi būti surenkamas atskirai nuo buitinių atliekų, kaip nustatyta kiekvienoje regione. Šiuo simboliu paženklinyti produktai neturi būti išmetami kartu su buitiniomis atliekomis.

**LV** Šis simbols norāda, ka ES valstīs šo produktu jāievāc atsevišķi no mājsaimniecības atkritumiem, kā noteikts katrā reģionā. Produkts ar šo simbolu nedrīkst izmest kopā ar mājsaimniecības atkritumiem.

**SI** Ta simbol označuje, da je treba proizvod v državah EU zbirati ločeno od gospodinjskih odpadkov, tako kot je določeno v vsaki regiji. Proizvoda s tem znakom ni dovoljeno odlagati skupaj z gospodinjskimi odpadki.

**GR** Το σύμβολο αυτό υποδηλώνει ότι στις χώρες της Ε.Ε. το συγκεκριμένο προϊόν πρέπει να συλλέγεται χωριστά από τα υπόλοιπα οικιακά απορρίμματα, σύμφωνα με όσα προβλέπονται σε κάθε περιοχή. Τα προϊόντα που φέρουν το συγκεκριμένο σύμβολο δεν πρέπει να απορρίπτονται μαζί με τα οικιακά απορρίμματα.

**CE** This product complies with the requirements of EMCD 2014/30/EU, LVD 2014/35/EU and Electromagnetic Compatibility Regulations 2016, Electrical Equipment (Safety) Regulations 2016.



---

For the U.K.:

**IMPORTANT:**

As the colors of the wires in the mains lead of this apparatus may not correspond with the colored markings identifying the terminals in your plug, proceed as follows:

The wire which is colored GREEN-AND-YELLOW must be connected to the terminal in the plug which is marked by the letter E or by the safety earth symbol ⊕ or colored GREEN or GREEN-AND-YELLOW.

The wire which is colored BLUE must be connected to the terminal which is marked with the letter N or colored BLACK.

The wire which is colored BROWN must be connected to the terminal which is marked with the letter L or colored RED.

For additional safety, all externally accessible metal parts (such as headphones, Aux-in/out, MIDI, toe pistons, etc.) are floating from safety earth.

THIS APPARATUS MUST BE EARTHED

THE WIRES IN THIS MAINS LEAD ARE COLOURED IN ACCORDANCE WITH THE FOLLOWING CODE.

GREEN-AND-YELLOW: EARTH, BLUE: NEUTRAL, BROWN: LIVE

**WARNING:**

---

仅适用于海拔2000m以下地区安全使用。



《2000m تەڭ يۇرتتا بىر تەرىپىدە بىر قىسىم ئورمان ۋە ئورماندىن ئىبارەت بىر تەرىپىدە بىر قىسىم...》

“تۇرۇشلۇق رايونلاردا 2000 مېتىر تۆۋەن رايونلاردا بىخەتەر ئىشلەتكىلى بولىدۇ”

Dan hab yungh youq gij digih haijbaz 2000m doxroengz haenx ancienz sawjyungh.

دېڭىز يۈزىدىن 2000 مېتىر تۆۋەن رايونلاردا بىخەتەر ئىشلەتكىلى بولىدۇ

---









